



419 N. Curtis Boise, ID 83706 208-429-0026

Laminated AFO Workorder Rev. 06092022

Received: _____ By: _____
Rush Charge Lab use only

PO#: _____ Date Needed: _____



Patient Information

Name: _____
Left Weight: _____
Right Activity Level: _____
Bilateral



Practitioner: _____
Company: _____ Ship to (if different): _____
Address: _____
City, State, Zip: _____
Email: _____ Shipping Method: _____
Phone: _____ UPS/Fedex #: _____

Prep Fill/Modify are typically 1 unit for pediatric, 2 for adult, and 3 for large AKs/hips/chest
FF Fill
FM Modify
Adjust

Foot Plate/Trimlines

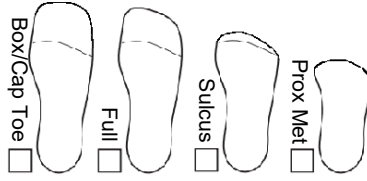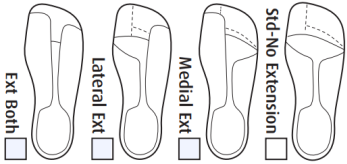

Inner Boot/Trimlines

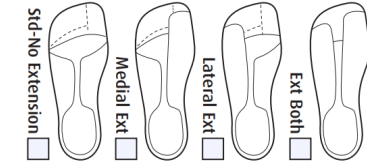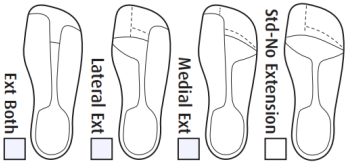

AFO Type

- FASL Solid Ankle
FAAT Art. Ankle
FABV Boise Bi
FPFA Partial Foot

Lamination

- Light
Standard
FHDL Heavy Duty

Finish

- Braid
Black
Solid
Beige
Fabric
White
Other

Pigment

Inner Boot

- Yes FAIB No
PolyPro

Plastic

- CoPoly
Optiflex
MPE

Thickness

- 3/32 1/8
5/32 3/16

Boot Trimline

- 3/4
Total Contact

Joints

Lateral

- ZTJ Tamarack
Dorsi
Free Motion
ZBD Double Action
Spring
Pin

Medial

- ZTJ Tamarack
Dorsi
Free Motion
ZBD Double Action
Spring
Pin

90° Stop

- Yes
No

Straps

- ZS1 Velcro 1"- 1.5"
ZSHD1 Dacron 1"- 1.5"
ZSV1 Velstretch 1"- 2"
Black
Beige
White
Other

Attach Straps

- Yes No

Ant. Shell


- FASS Simple Shell
FAAS Molded Shell

Quality Assurance

- Smooth edges
Symmetrical trim
Pads glued/Incl.
Straps On/Incl.
Strap placement
Joint Alignment
Comp. Loctited
All parts Incl.
Proj. tote cleared
Engraved P.O.
Mods
Pull
Finish
QA
Finish Date

Modifications

Standard modifications are no reductions on AFOs with 1/8" ankle buildup

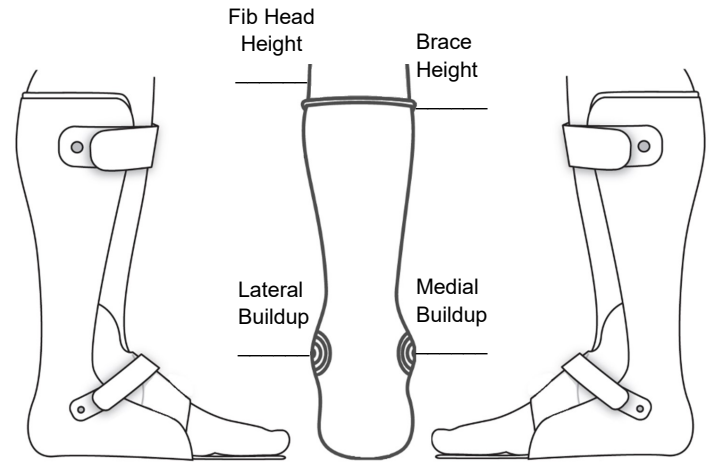

Mod Notes

Insole/Support

- ZPIS Pelite Insole (per layer)
Neutral to Bench
Distance from Neutral

Add. Padding

Thickness

Pad Type

- Ant. Ankle ZAA
Ankle
Planar
Calf
Other:
Puff
Plast
P.Cell
Aliplast

Pad Color

- Black Other:

Hourly Labor FHL

Additional Notes

Send Cast/Parts to: Coyote, 419 N. Curtis Rd., Boise, ID 83706