


Parts included

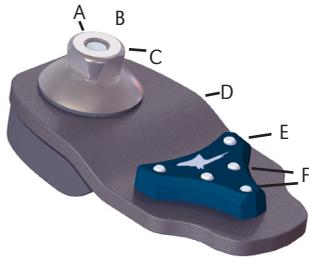

- A Titanium Pyramid
- B Machined Washer
- C Pyramid Bolt
- D Keel
- E Cleat Bracket
- F Screws

Excepts 2 and 3 hole cleats
 3- 16mm screws for attaching plate to keel
 3- 20mm screws for attaching 2 hole cleats
 3- 22mm screws for attaching 3 hole cleats

- | | |
|--------------------------------|----------------------------------|
| EN Instructions for Use | NL Gebruiksaanwijzing |
| DE Gebrauchsanweisung | PT Instruções de Utilização |
| FR Notice d'utilisation | PL Instrukcja użytkowania |
| ES Instrucciones para el uso | CS Návod k použití |
| IT Istruzioni per l'uso | TR Kullanım Talimatları |
| NO Bruksanvisning | RU Инструкция по использованию |
| DA Brugsanvisning | JA 取扱説明書 |
| SV Bruksanvisning | ZH 中文说明书 |
| EL Οδηγίες Χρήσης | KO 사용 설명서 |
| FI Käyttöohjeet | |

www.coyote.us/instructions



FB1 Cyclone™ Instructions Coyote Bike Foot

2-year warranty against manufacturer defects, excessive wear or breakage.

Patent Pending
 External Prosthetic Components



Advena Limited
 Tower Business Centre
 2nd Flr, Tower Street
 Swatar, BKR 4013
 Malta
 FB1.revA.11302022



Manufactured by Coyote®
 419 N. Curtis Rd., Boise, Idaho 83706
 (208) 429-0026 | www.coyote.us



Lower Extremity Prosthesis

14mm M-L adjustment

Device is intended for activity levels K3-K4

L-Code – L5999

Sizes Available: One size fits all.

The device is only for use by a certified practitioner and the end user.

Product Description

The Coyote Cyclone™ Bike Foot (FB1) was designed for K3-K4 level ambulators who desire a light weight, durable, and rigid foot. It is designed to give optimal power stroke, fit and alignment for cycling.

The Cyclone™ Bike Foot was designed without compromising durability and to minimize foot weight. While pedaling, the Cyclone™ gives unmatched energy transfer. The short foot length design increases pedal stroke efficiency.

The innovative design eliminates energy lost to weight caused by a foot shell and shoe. It also eliminates energy loss due to shoe and foot shell flex.

The adjustable pyramid allows the foot to be either right or left. The cleat bracket can be used with two or three hole cleats.

Technical Specifications

Build Height: 1.75"

Product weight: 215g (without cleat)

Maximum user weight: 265 lbs.

Indications for Use

Lower limb amputation

Contraindications and Precautions

Conditions in a recipient that increases the risk for a serious adverse reaction are unknown.


Intended Use

This is a non-invasive reusable device designed for single patient use. The foot is designed for bicycling and clipping into a pedal with minimal walking.

The Cyclone Bike foot parts have not been torqued and have not had Loctite® applied.

Once the foot has been adjusted, and before using the bike foot, make sure to torque and Loctite® all parts.

Check "Pyramid Medial/Lateral Adjustment" section for torque settings and always apply Loctite® Blue 242 to threads.

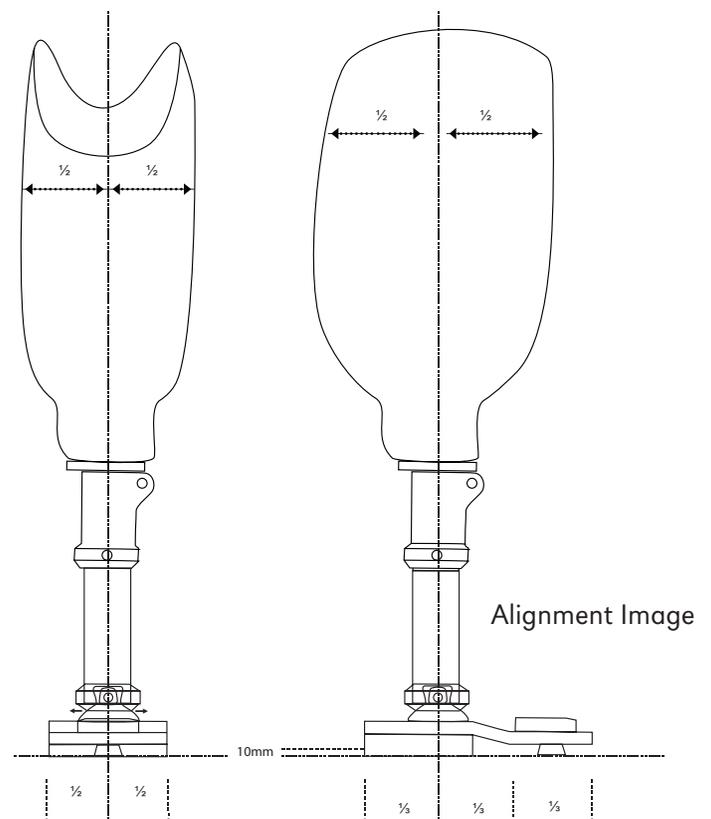

Foot Cover

The product is not designed to not to be used with a foot cover or shoe.

2-year warranty against manufacturer defects, excessive wear, or breakage.

SAFETY

Warnings

Coyote products are designed and tested to meet industry standards and to match Coyote’s own standards where an industrial standard does not apply.

The device should be used with the appropriate adapters.

Excessive strain on the product can increase risk of failure. This includes improper use and heavy loads which might include repetitive excess weight loads.

Damage to the product and internal parts.

If you notice a change in the products functionality, check the product for damage.

A new noise that starts, changes in gait, changes in alignment, malfunction, or functional loss, are all examples of possible damage.

If changes occur, discontinue using the prosthetic and have it inspected by a qualified professional.

Pyramid Medial / Lateral Adjustment




1 The pyramid adjustment slot on top of keel gives the pyramid 14 mm of slide from side to side. This makes it possible for the foot to be adjusted for a right or left pedal.



2 The pyramid has set screws extending from the bottom to help hold alignment and prevent rotation.



3 The pyramid can be adjusted to the bicyclists preference. If the pyramid is slid to the left, it is for the right foot. If the pyramid is slid to the right, it can be used for the left foot, although the slide allows for any type of alignment given the patients’ needs or riding style. Make sure the set screws are in the keel slots before tightening the bolt securing the pyramid into position. Always apply Loctite® Blue 242 to threads of the bolt and torque the bolt head to 40 Nm.

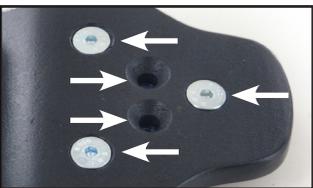

4 The Cyclone can be used with two or three hole bike cleats. Always apply Loctite® Blue 242 to threads and torque M10 (6mm hex drive), M5 (3mm hex drive) screws to 10 Nm.

5 Once you have definitive alignment of the pyramid and bracket Loctite® all screws into position with Loctite® Blue 242.

Always, *LOCTITE*
and torque to manufacturer specifications.

Use under adverse environmental conditions

Product damage may increase the risk of injury.

Adverse environmental conditions may damage the prosthetic.

If adverse conditions have occurred check for any damage.

If damage has occurred, if you feel damage may have occurred, or if you notice a change in stiffness, or loss of support quit using the product.

Have the product cleaned, repaired, needed parts replaced and inspected by a qualified individual or facility.

The device is water resistant, all parts are stainless steel, titanium, or composite. It is recommended if you have been in dust, sand, highly hygroscopic particles (e.g. talcum), saltwater, or pool water the foot should be properly rinsed with fresh water and dried, inspect and remove sand and debris.

Environmental Conditions

Environmental Operating Temperature: -15°C (-5°F) to 50°C (122°F)

Shipping and Storage Temperature: -10°C (-4°F) to 70°C (158°F)

Yearly safety checks are recommended.

The Cyclone Bike foot parts have not been torqued and have not had Loctite® applied. Once the foot has been adjusted and before using the bike foot, make sure to torque and Loctite® all parts. Check “Pyramid Medial/Lateral Adjustment” section for torque settings and always apply Loctite® Blue 242 to threads.

Foot	Coyote	Foot	Category	Size	Side	Pyramid
Cyclone		F	B	1	—	—

Part Number: Cyclone - FB1

Choose Foot Cyclone Bike Foot (FB1) Side Adjustable to Left or Right
 Choose Category (B) Bike Pyramid Titanium
 Size One Size



To order, contact Coyote® or your favorite distributor.

If you have any questions, please call Coyote at 208-429-0026 or email us at coyote@coyoteprothetics.com

www.coyote.us